

## NRC Publications Archive Archives des publications du CNRC

### Report on inter-laboratory comparison of guarded hot plate measurements

Salmon, D.; Silberstein, A.; Kumaran, M. K.

For the publisher's version, please access the DOI link below. / Pour consulter la version de l'éditeur, utilisez le lien DOI ci-dessous.

#### **Publisher's version / Version de l'éditeur:**

<https://doi.org/10.4224/20359196>

*Internal Report (National Research Council of Canada. Institute for Research in Construction); no. IRC-IR-653, 1993-12*

#### **NRC Publications Archive Record / Notice des Archives des publications du CNRC :**

<https://nrc-publications.canada.ca/eng/view/object/?id=920c9733-3f90-46c1-a3f2-6213a419b8e3>

<https://publications-cnrc.canada.ca/fra/voir/objet/?id=920c9733-3f90-46c1-a3f2-6213a419b8e3>

Access and use of this website and the material on it are subject to the Terms and Conditions set forth at

<https://nrc-publications.canada.ca/eng/copyright>

READ THESE TERMS AND CONDITIONS CAREFULLY BEFORE USING THIS WEBSITE.

L'accès à ce site Web et l'utilisation de son contenu sont assujettis aux conditions présentées dans le site

<https://publications-cnrc.canada.ca/fra/droits>

LISEZ CES CONDITIONS ATTENTIVEMENT AVANT D'UTILISER CE SITE WEB.

**Questions?** Contact the NRC Publications Archive team at

PublicationsArchive-ArchivesPublications@nrc-cnrc.gc.ca. If you wish to email the authors directly, please see the first page of the publication for their contact information.

**Vous avez des questions?** Nous pouvons vous aider. Pour communiquer directement avec un auteur, consultez la première page de la revue dans laquelle son article a été publié afin de trouver ses coordonnées. Si vous n'arrivez pas à les repérer, communiquez avec nous à PublicationsArchive-ArchivesPublications@nrc-cnrc.gc.ca.

SER  
TH1  
R427  
BLDG  
no. 653  
December  
1993



**National Research  
Council Canada**

**Conseil national  
de recherches Canada**

Institute for  
Research in  
Construction

Institut de  
recherche en  
construction

# **NRC-CNRC**

## **Report on Inter-Laboratory Comparison of Guarded Hot Plate Measurements**

by David Salmon, Anne Silberstein and Kumar Kumaran

**Internal Report No. 653**

Internal report : Institute  
\_\_Bev Creighton ANALYSE

**Date of Issue: December 1993**

**ANALYZED**

CISTI/ICIST NRC/CNRC  
IRC Ser  
Received on: 01-14-94  
Internal report : Institute  
for Research in  
Construction Canada

This is an internal report of the Institute for Research in Construction. Although not intended for general distribution, it may be cited as a reference in other publications.

**Canada**

13389870

# **REPORT ON INTER-LABORATORY COMPARISON OF GUARDED HOT PLATE MEASUREMENTS**

David Salmon  
Division of Quantum Metrology  
National Physical Laboratory  
Teddington, Middlesex TW11 0LW  
England

Anne Silberstein  
Isover Saint-Gobain  
CRIR  
Centre de Recherches et de Developpement  
60290 Rantigny  
France

**ANALYZED**

Kumar Kumaran  
Building Performance Laboratory  
Institute for Research in Construction  
National Research Council Canada  
Ottawa Ontario K1A 0R6  
Canada

# REPORT ON INTER-LABORATORY COMPARISON OF GUARDED HOT PLATE MEASUREMENTS

## INTRODUCTION

The guarded hot-plate apparatus is the primary standard for the measurement of thermal conductivities of thermally insulating materials. Standard test procedures using the guarded hot plate are prescribed by ASTM and ISO. In principle, the values of thermal conductivities determined using a well-designed apparatus could be accurate to between 0.5% and 1 %. But experience shows that the design, construction and operation of a guarded hot plate apparatus are very challenging tasks and it is not always possible to attain the highest theoretical accuracy. For example, the ISO Standard document No. 8302:1991(E) quotes the following limit values:

Expected guarded hot plate method accuracy (at room temperature) 2 %

Expected guarded hot plate method accuracy (full temperature range) 5 %

The work reported here was undertaken to compare the results obtained using four guarded hot plate apparatus that differ in design and modes of operation and to establish the agreement between the British, French and Canadian national standards.

## WORK PLAN

The work plan included the following steps:

1. From stocks of 25 mm and 75 mm thick glass fiber insulation of well-characterised bulk density, thickness and thermal resistance, select matched pairs of test specimens of dimensions 600 mm x 600 mm.
2. Each of the participating laboratories should test the same matched pairs on their apparatus to determine the apparent thermal conductivity of the insulation as a function of temperature, in the range 0 ° C to 40 ° C.

## TEST SPECIMENS

Three pairs of test specimens were included in the work. Two pairs were selected from NPL and one pair from IRC. All these pairs had well-characterised thermal conductivities and the physical characteristics, as listed below.

### *The NPL Specimens*

The two pairs of NPL specimens were made out of four slabs with coding, LA4, LA5, LA6 and LA8. The physical characteristics of the slabs, as shown in Table 1, were

determined at IRC. The properties of LA4 and LA6 match well and so do those of LA5 and LA8. Hence, the two pairs of specimens were matched for thermal conductivity measurements as:

Specimen pair 1, referred to as NPL1, consists of LA4 and LA6 and

Specimen pair 2, referred to as NPL2, consists of LA5 and LA8.

#### *The IRC Specimens*

One pair of slabs from IRC, coded as 364-146-A and B, formed yet another pair of test specimens, referred to as IRC1. The properties of these slabs are also given in Table 1.

Table 1. The physical properties of individual slabs used to make three pairs of test specimens. The thermal resistances were determined using a heat flow meter apparatus at a mean specimen temperature of 24 °C

Specimen code	Thickness mm	Bulk density kg.m <sup>-3</sup>	Thermal resistance m <sup>2</sup> .K.W <sup>-1</sup>
Specimen pair NPL1			
LA4	74.64	53.5	2.37
LA6	74.48	52.3	2.36
Specimen pair NPL2			
LA5	74.62	44.3	2.31
LA8	74.48	44.2	2.30
Specimen pair IRC1			
364-146-A	26.09	53.2	0.822
364-146-B	26.09	53.4	0.818

## TEST APPARATUS

All the apparatus used in this work are guarded hot plate apparatus and they are all based on the same principle. All hot plates have a square geometry. However, as summarised below, there are some differences in the details of design and methods of operation.

#### *The NPL 610 mm guarded hot plate/ heat flow meter apparatus*

The apparatus has been designed to measure the thermal conductivity of single specimens from 30 mm to 300 mm thick in the temperature range 10 °C to 30 °C and to operate either in the primary mode as a conventional guarded hot plate or in a secondary mode using a heat flow meter. A 250 mm square heat flow meter is embedded in the central area of a 610 mm square by 5 mm thick "paxolin" sheet which is bolted to the lower surface of the cold plate assembly. It can be used either to check that linear heat flow has been established in thick specimens when measurements are carried out using the apparatus as a guarded hot plate or, to measure the mean heat flux through the specimen when the apparatus is operated as a heat flow meter apparatus. Specially designed

copper-plated printed circuit boards have been developed as heating elements for the main heater plate, the auxiliary guard, and the cold plate of the apparatus, to provide the uniform heating necessary to produce large isothermal surfaces. The metering area is  $\approx 300 \text{ mm} \times 300 \text{ mm}$ . A linear temperature gradient edge-guard consisting of four thin stainless steel sheets is located parallel to and 25 mm from the specimen edges. One end of each sheet is clamped to the cold plate and the other is controlled at the temperature of the hot plate to produce a linear temperature gradient matching that in the specimen. This additional guard ensures that there is no heat-flux across the boundaries of the specimen. The height of the cold plate assembly above the main hot plate is adjusted by a motor driven mechanism in which the plates are kept parallel by rollers bearing on a long chrome-plated cylinder. Specimen thickness is derived from the output of a linear voltage displacement transducer. A line diagram of the apparatus is given in Figure 1.

#### *The CRIR(ISOVER SAINT-GOBAIN) guarded hot plate apparatus*

The CRIR guarded hot plate apparatus is a "one-specimen" apparatus, that functions in a bi-guarded, horizontal configuration. Plate dimensions are 610 mm x 610 mm with a metering area of 250 mm x 250 mm. The metering area is surrounded by two guards. The plate assembly rests in a temperature and humidity controlled atmosphere. The imbalances between the metering area and the first guard and that between the first and the second guard are controlled using thermopiles with 100 and 200 thermocouple junctions respectively.

#### *The IRC guarded hot plate apparatus*

There are two apparatus at IRC, one of which conforms to ASTM Standard C 177. The 610 mm X 610 mm hot plate has one auxiliary guard. The metering area is 300 mm x 300 mm. It is operated in the two-sided mode, in the vertical configuration. This apparatus is referred to as IRC OLD apparatus. The hot plate of the second apparatus, referred to as IRC NEW apparatus, is identical to that of the CRIR apparatus in design. However, the metering area and the guards are held together using foamed-in-place polyurethane insulation and avoid any thermal bridging due to physical connections with lower thermal resistance. The apparatus is designed for use in the one-sided as well as two-sided modes, in either a vertical configuration or a horizontal configuration. The measurements reported here were performed in the two-sided mode, in the vertical configuration.

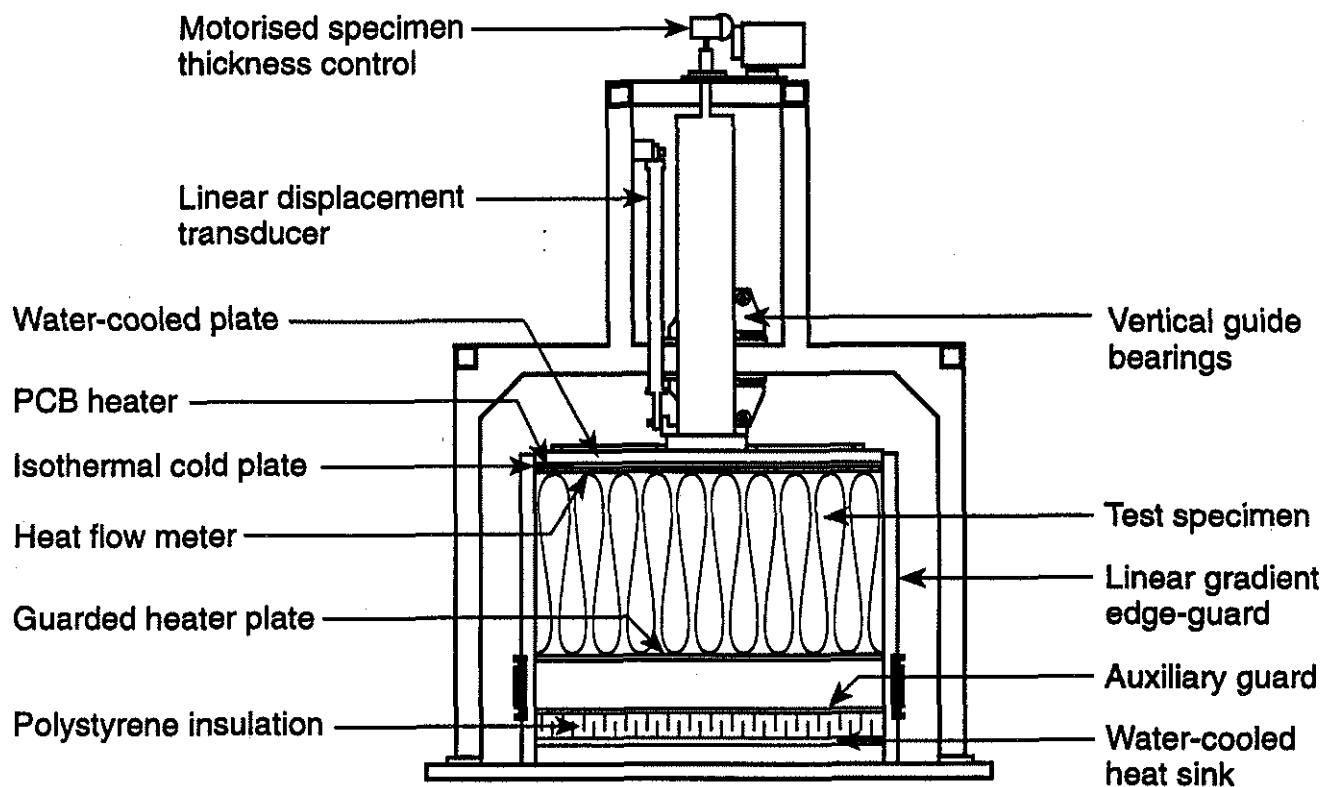


Figure 1. Schematic drawing of the 610 mm guarded hot plate/heat flow meter apparatus at the National Physical Laboratory, United Kingdom.

## RESULTS ON THE SPECIMEN NPL1

The test results on the thermal conductivity of NPL1 reported from the three participating laboratories are listed in Table 2 and are plotted in Figure 2.

Table 2. Experimental results on the thermal conductivity of NPL1 at various temperatures; the data referred to as "fitted" are those calculated from a linear equation generated using all the available data.

Temperature ° C	Thermal conductivity W.m <sup>-1</sup> .K <sup>-1</sup>					
	NPL	CRIR	IRC-OLD	IRC-NEW	Fitted	% Deviation
8.85	0.03025				0.03012	0.5
8.86	0.03020				0.03012	0.3
23.45	0.03218				0.03206	0.4
23.49	0.03201				0.03207	0.2
30.54	0.03302				0.03300	0.1
36.84	0.03378				0.03384	0.2
36.85	0.03400				0.03885	0.5
1.5		0.0290			0.02914	0.5
2.0		0.0292			0.02920	0.0
4.7		0.0295			0.02956	0.2
9.5		0.0302			0.03020	0.0
9.5		0.0303			0.03020	0.3
24.0		0.0325			0.03213	1.1
24.0		0.0318			0.03213	1.0
29.3		0.0328			0.03284	0.1
29.3		0.0329			0.03284	0.2
39.6		0.0344			0.03421	0.6
40.2		0.0344			0.03429	0.3
9.98			0.03036		0.03027	0.3
23.71			0.03209		0.03209	0.0
40.08			0.03424		0.03428	0.1
11.34				0.03040	0.03045	0.2
15.95				0.03103	0.03106	0.1
21.02				0.03172	0.03174	0.1
26.04				0.03226	0.03241	0.5
30.77				0.03283	0.03304	0.6
35.97				0.03348	0.03373	0.7

Note: NPL and ISOVER values measured at 75 mm nominal thickness for each specimen of the pair.

# RESULTS ON NPL1

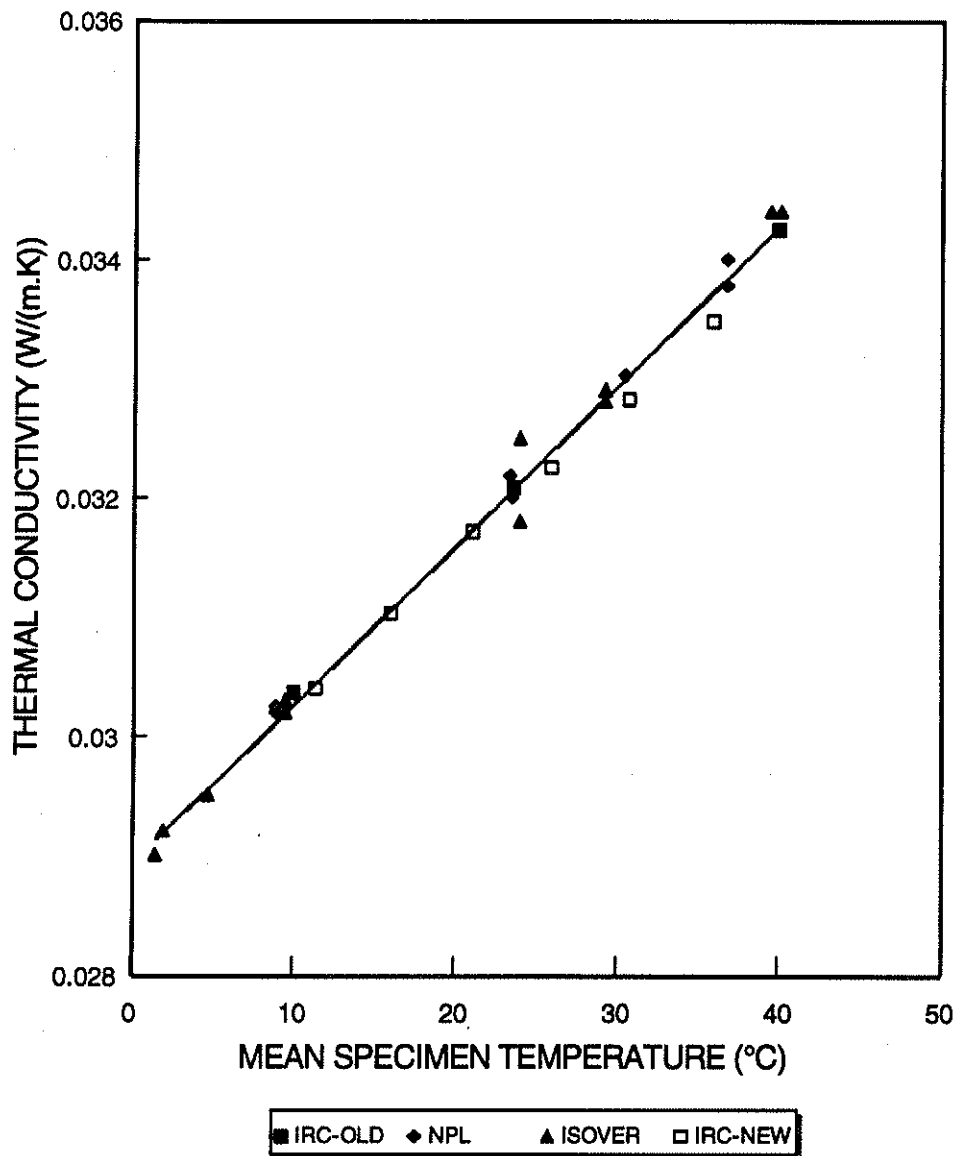


Figure 2. Experimental data, listed in Table 2, from four different guarded hot plate apparatus; the solid line is the best fit obtained from a linear regression that included all the experimental data.

## RESULTS ON THE SPECIMEN NPL2

The test results on the thermal conductivity of NPL2 reported from the three participating laboratories are listed in Table 3 and are plotted in Figure 3.

Table 3. Experimental results on the thermal conductivity of NPL2 at various temperatures; the data referred to as "fitted" are those calculated from a linear equation generated using all the available data.

Temperature ° C	Thermal conductivity W.m <sup>-1</sup> .K <sup>-1</sup>					
	NPL	CRIR	IRC-OLD	IRC-NEW	Fitted	% Deviation
8.79	0.03076				0.03083	0.2
9.02	0.03099				0.03086	0.4
23.45	0.03291				0.03293	0.1
30.76	0.03426				0.03398	0.8
36.86	0.03478				0.03485	0.2
37.05	0.03505				0.03488	0.4
1.8		0.0297			0.02983	0.5
1.8		0.0300			0.02983	0.6
9.5		0.0307			0.03093	0.8
9.5		0.0312			0.03093	0.9
24.0		0.0334			0.03301	1.2
24.4		0.0331			0.03306	0.1
29.3		0.0338			0.03377	0.1
30.0		0.0339			0.03387	0.1
39.6		0.0354			0.03524	0.5
39.6		0.0352			0.03524	0.1
10.47			0.03098		0.03107	0.3
24.15			0.03291		0.03303	0.4
39.80			0.03516		0.03527	0.3
10.83				0.03114	0.03112	0.1
15.14				0.03169	0.03174	0.2
20.04				0.03226	0.03244	0.6
24.97				0.03297	0.03315	0.5
29.14				0.03356	0.03374	0.5
34.13				0.03423	0.03446	0.7

Note: NPL and ISOVER values measured at 75 mm nominal thickness for each specimen of the pair.

## RESULTS ON NPL2

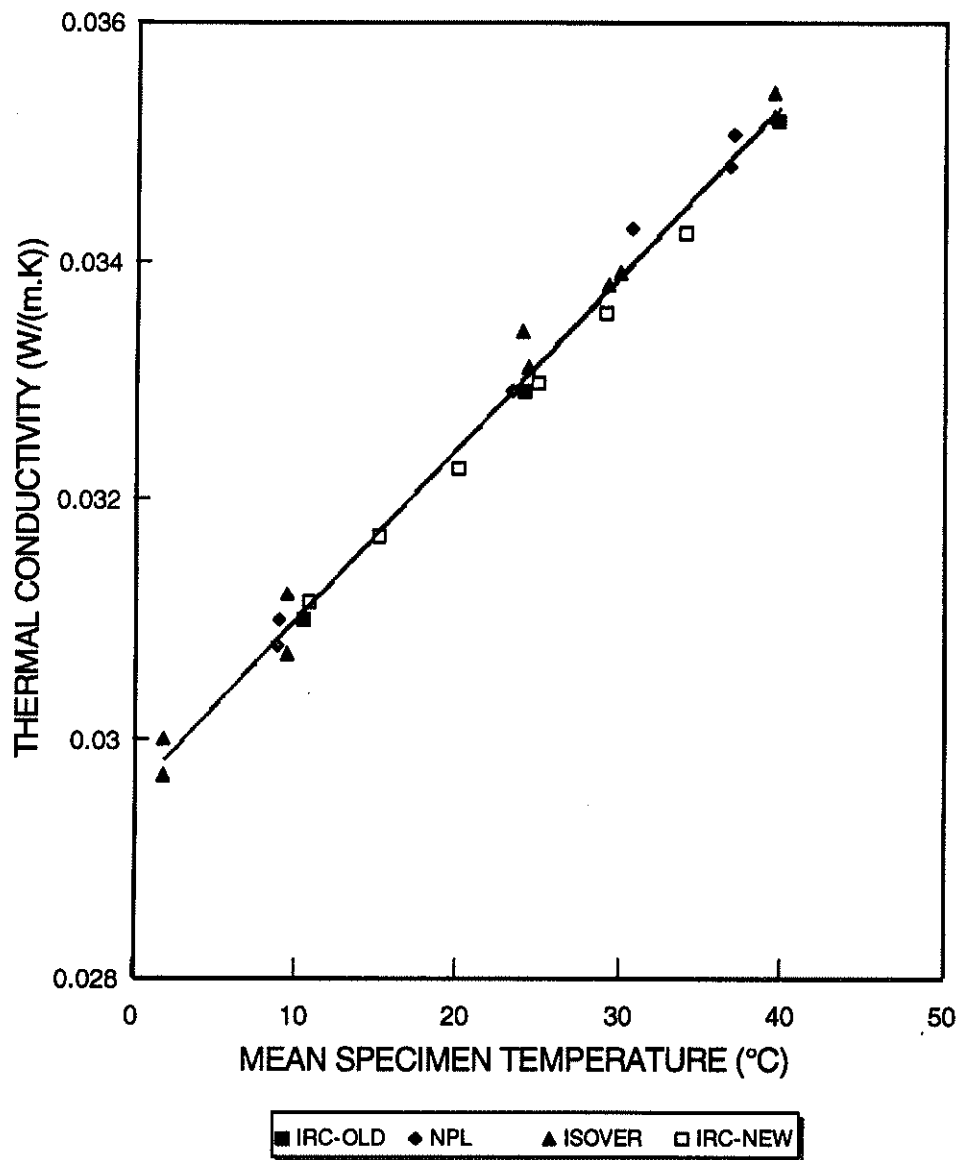


Figure 3. Experimental data, listed in Table 3, from four different guarded hot plate apparatus; the solid line is the best fit obtained from a linear regression that included all the experimental data.

## RESULTS ON THE SPECIMEN IRC1

The test results on the thermal conductivity of IRC1 reported from the three participating laboratories are listed in Table 4 and are plotted in Figure 4.

Table 4. Experimental results on the thermal conductivity of IRC1 at various temperatures; the data referred to as "fitted" are those calculated from a linear equation generated using all the available data.

Temperature ° C	Thermal conductivity W.m <sup>-1</sup> .K <sup>-1</sup>					% Deviation
	NPL	ISOVER	IRC-OLD	IRC-NEW	Fitted	
9.73	0.03091				0.03081	0.3
12.70	0.03128				0.03118	0.3
18.68	0.03206				0.03192	0.4
24.91	0.03290				0.03270	0.6
27.97	0.03325				0.03308	0.5
30.50	0.03358				0.03340	0.5
36.76	0.03442				0.03418	0.7
37.81	0.03456				0.03431	0.7
5.0		0.0305			0.03022	0.9
10.0		0.0311			0.03084	0.8
24.0		0.0328			0.03259	0.6
30.0		0.0337			0.03334	1.1
40.0		0.0348			0.03458	0.6
7.87			0.0302		0.03057	1.3
24.36			0.0322		0.03263	1.5
45.21			0.0351		0.03523	0.5
14.04				0.0310	0.03134	1.2
19.00				0.0317	0.03196	1.0
28.84				0.0328	0.03319	1.1
34.01				0.0335	0.03384	1.0
38.99				0.0342	0.03446	0.8

Note: NPL and ISOVER measurements were done on the specimens stacked together to form a single test specimen of 52 mm nominal thickness.

## RESULTS ON IRC1

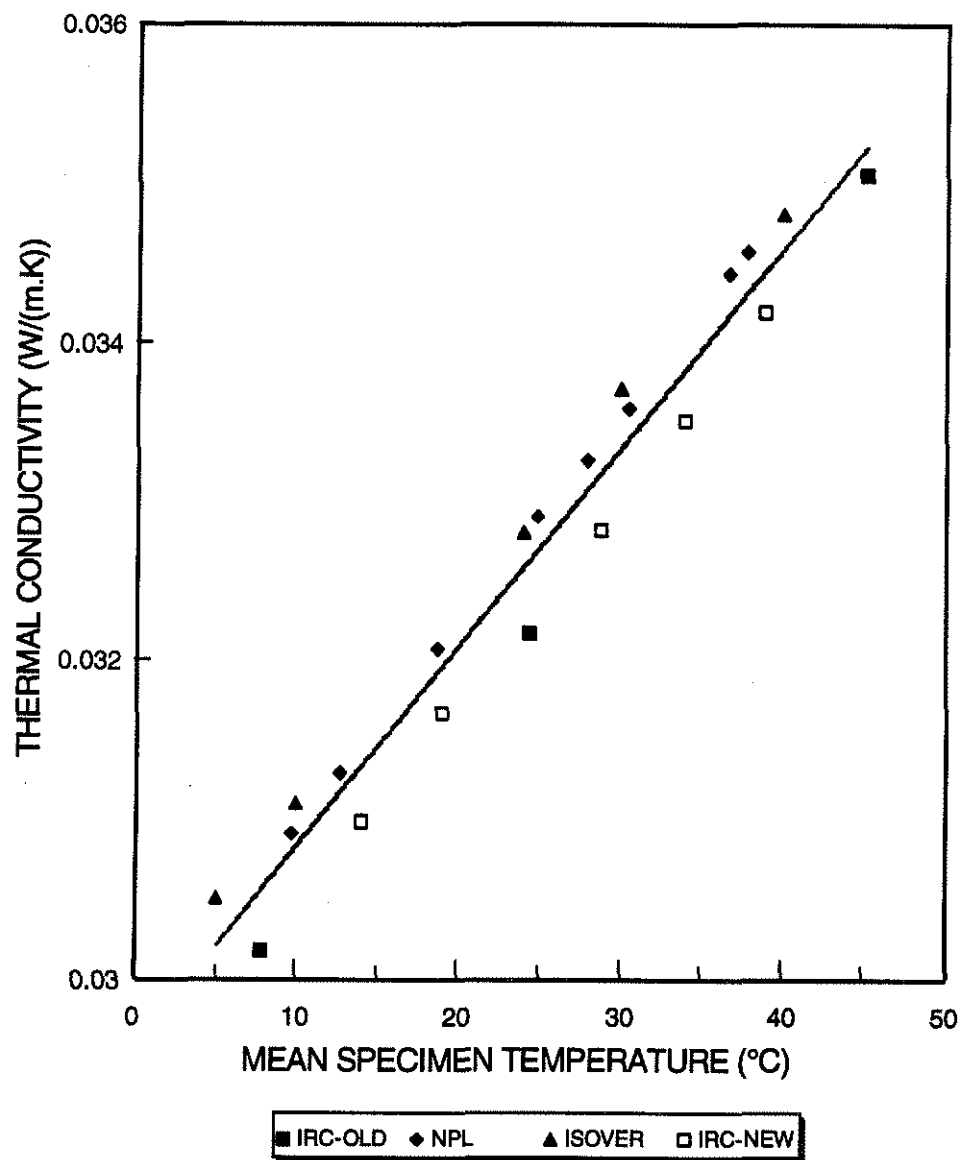


Figure 4. Experimental data, listed in Table 4, from four different guarded hot plate apparatus; the solid line is the best fit obtained from a linear regression that included all the experimental data.

## DISCUSSION

The results presented in Tables 2, 3 and 4 and plotted in Figures 2, 3 and 4 are the data obtained from the three participating laboratories. The thermal conductivity measurements were carried out on specimens of slightly different thicknesses depending on the amount of compression applied by each participating laboratory. The largest deviation from the nominal thickness of 25 mm and 75 mm was about 0.5 mm. However, it was not necessary to do a re-analysis of the results because the correction to the thermal conductivity would be quite small. Consider, for example, a 1 mm difference in thickness between the specimens in each apparatus, due to varying degree of compression. The effect on thermal conductivity should not be greater than 0.15 %, based on the available knowledge of the dependence of thermal conductivity of fibrous insulation on temperature and bulk density.

The Figures 2, 3 and 4 show that the largest difference between the four sets of measurements for all the three test specimens is about 2.2 %. In addition, the Tables 2, 3 and 4 show that the largest deviation of any datum from a least-squares fit is about 1.5 %.

## CONCLUSION

Three pairs of well-characterised specimens of glass fibre insulation of thicknesses 25 mm and 75 mm were used in the measurements of thermal conductivity, in the temperature range 0 °C and 40 °C, at the National Physical Laboratory (UK), ISOVER SAINT-GOBAIN (France) and the Institute for Research in Construction, National Research Council (Canada). The agreement between the three laboratories was within 2.2 %, the largest deviation from the least-squares fit to all the data being less than 1.5 %. This is outside the theoretical accuracy of 0.5 % to 1 % that one would expect from using a primary standard. But, as mentioned in the introduction, the design, construction and operation of guarded hot plates are very challenging tasks and consequently the agreement established between NPL, ISOVER and IRC can be considered very satisfactory. The agreement established in this work is much better than what is required by the ISO Standard on guarded hot plates.